

Fig. 1

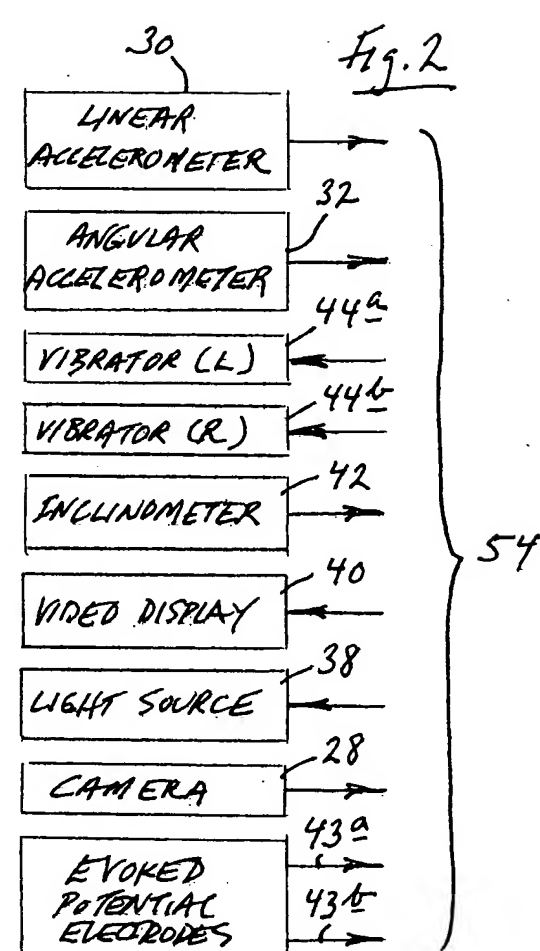
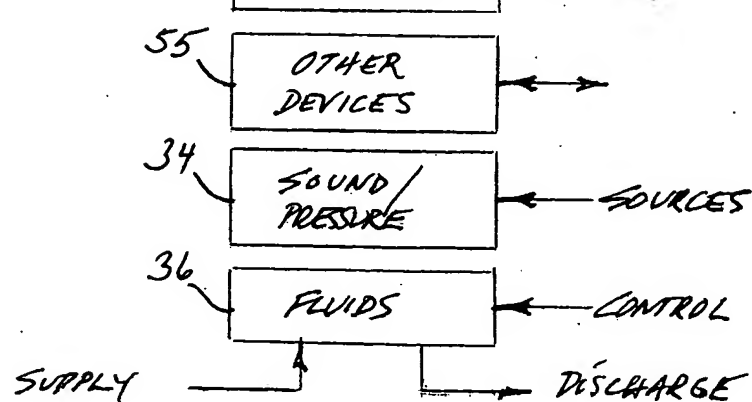
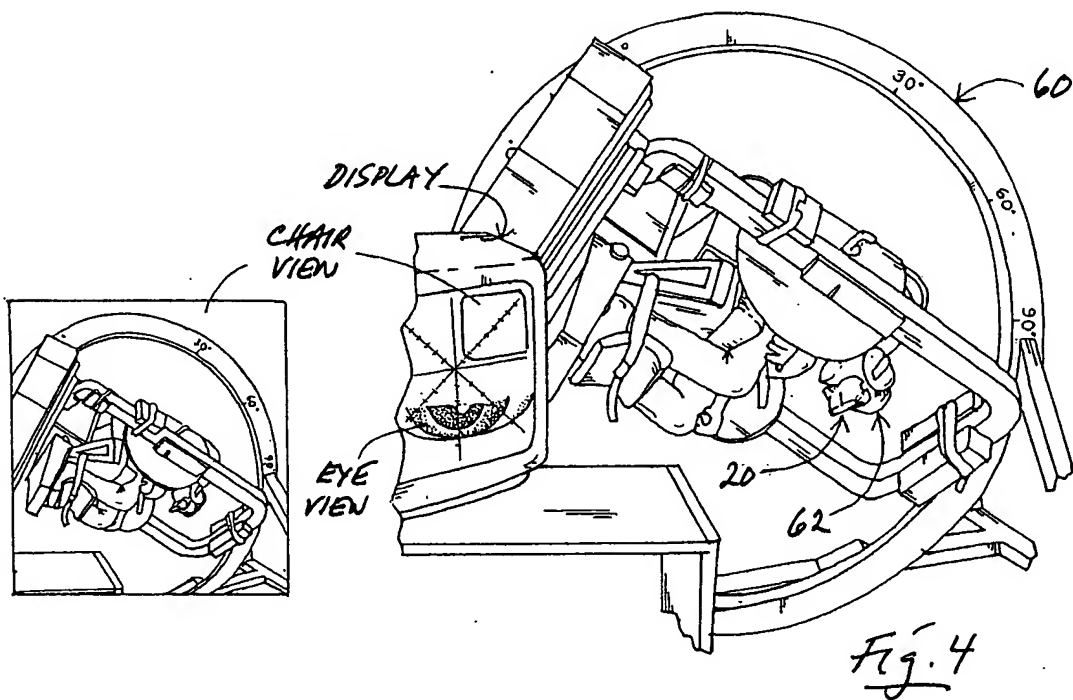
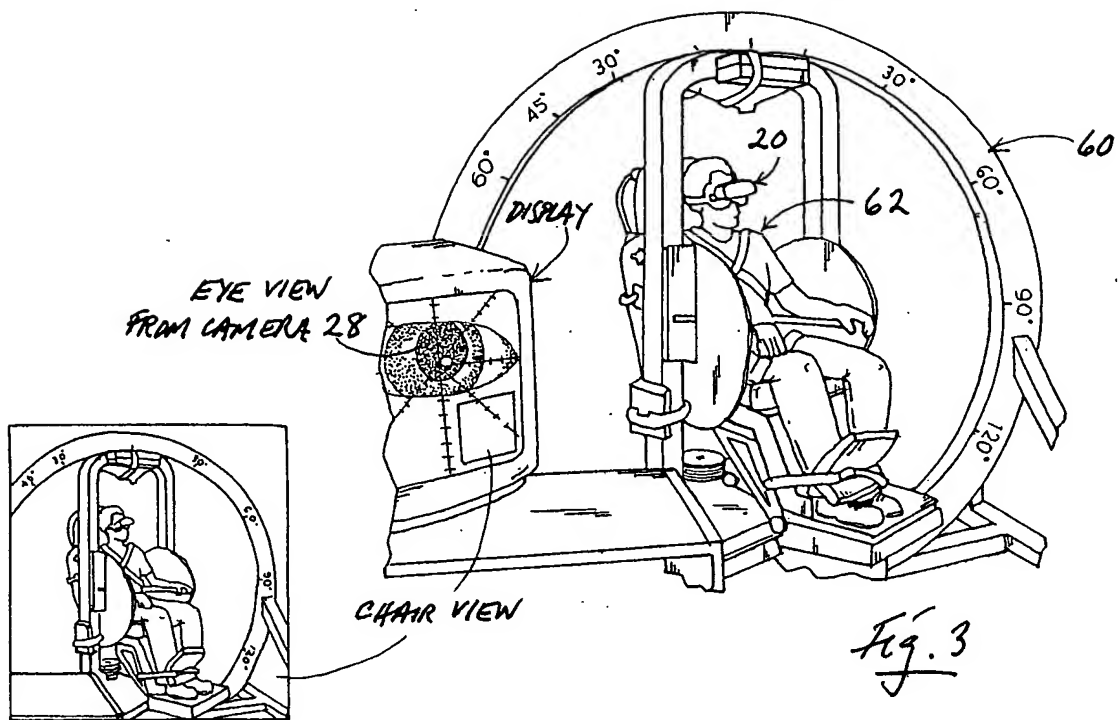
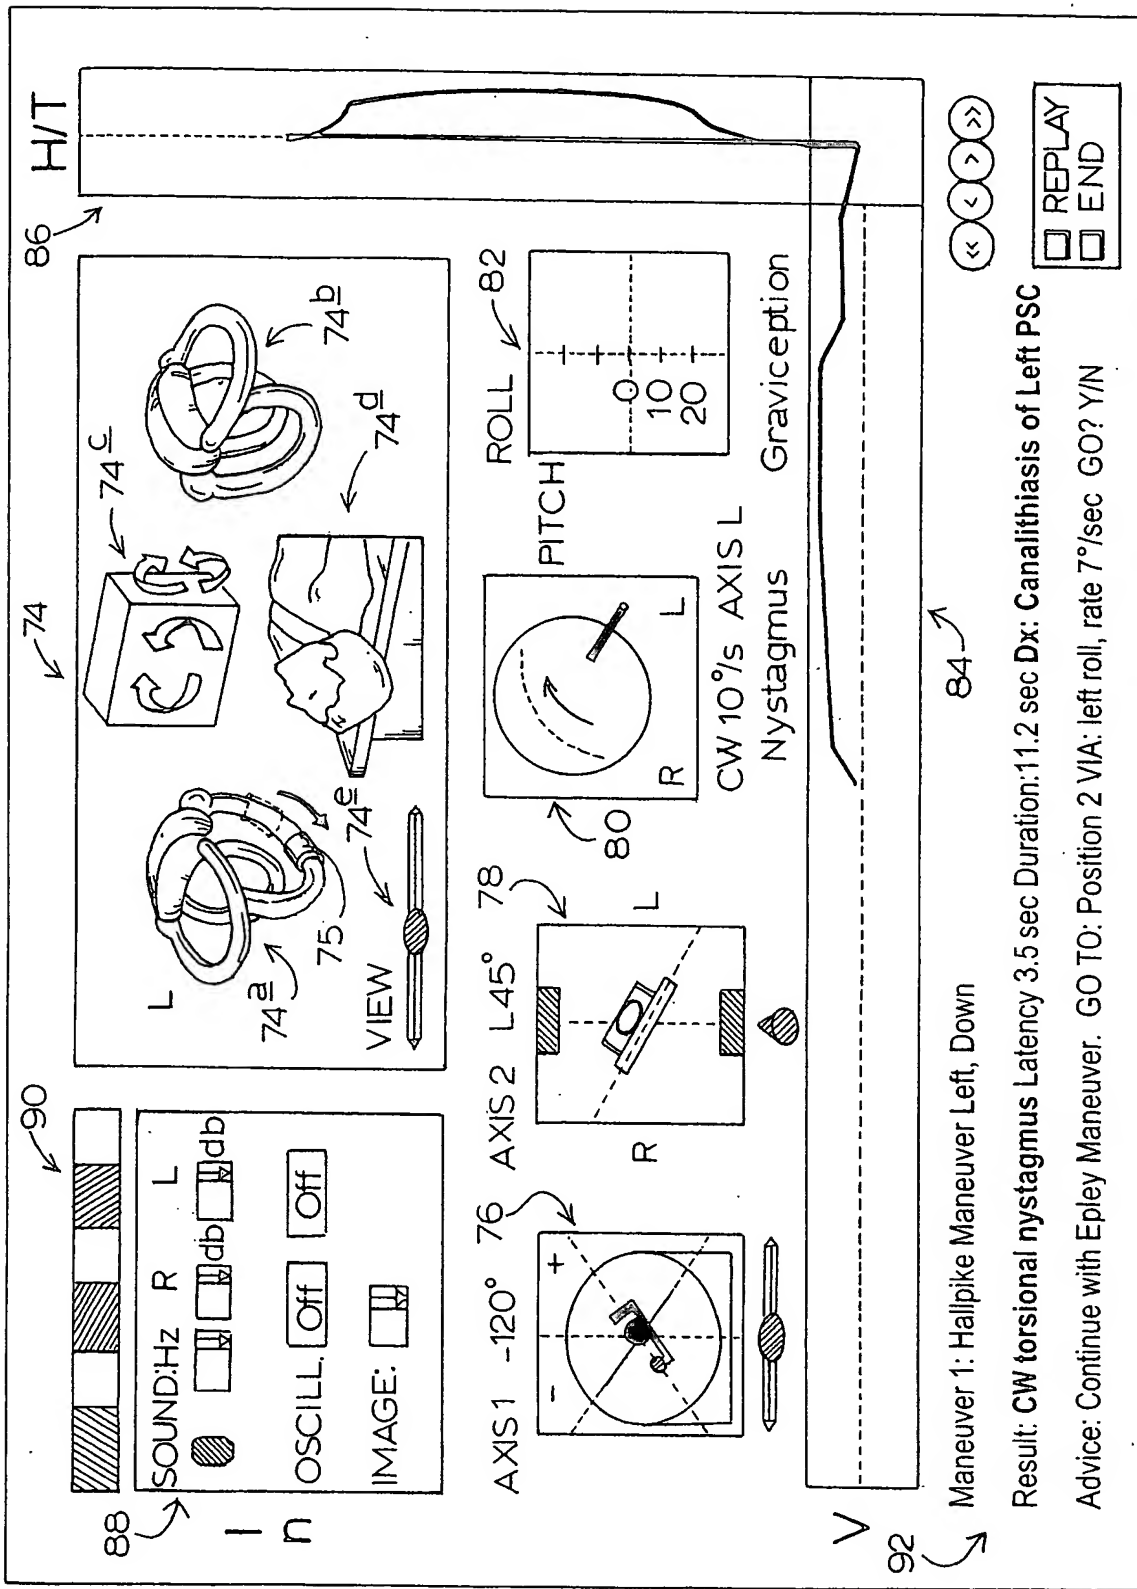





Fig. 2









*Fig. 5*

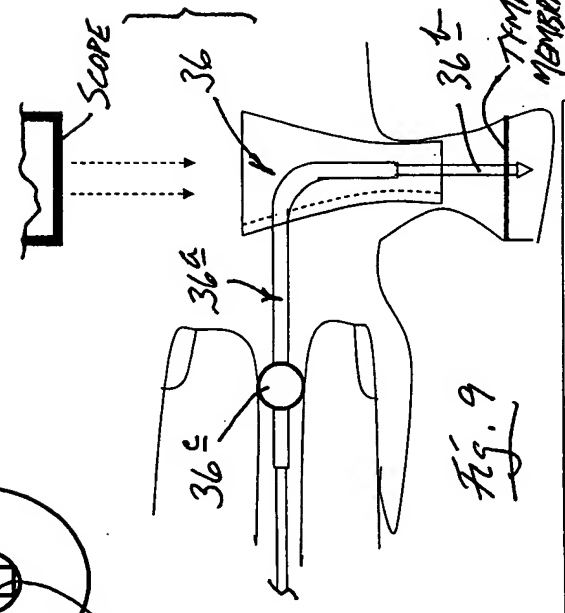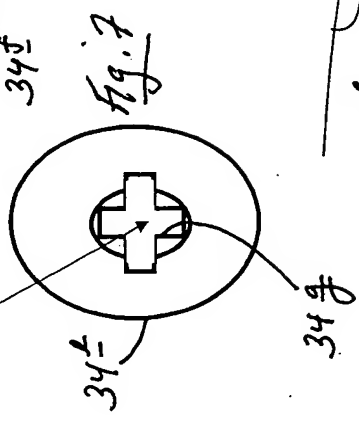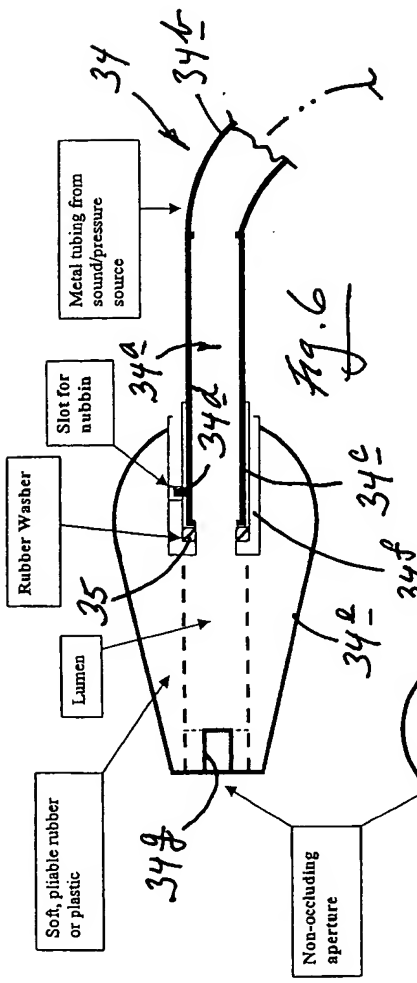

Insert trocar thru TM under direct view of scope, guiding by rolling bead between fingers. Handle fits thru slot in speculum.

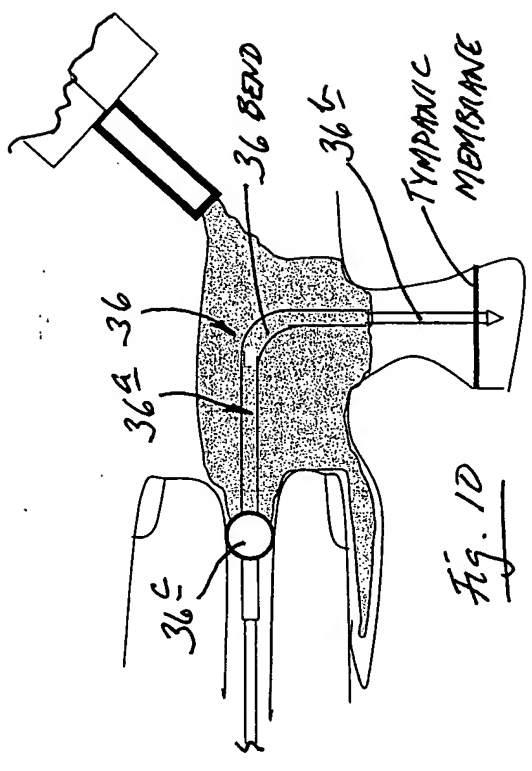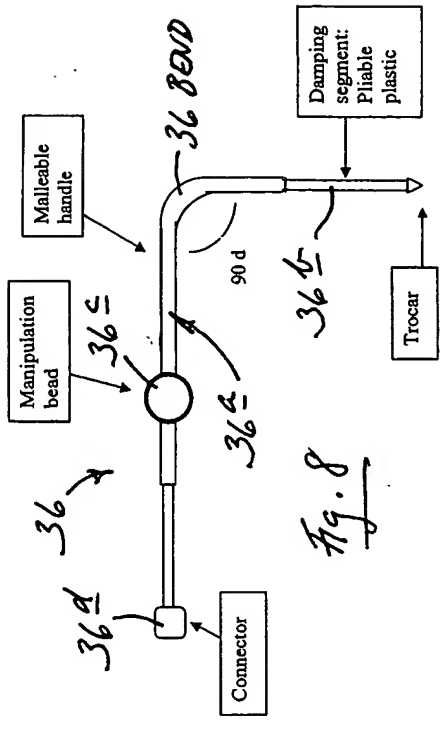

With fingers braced against head to stabilize trocar, remove speculum and inject molding material into area.

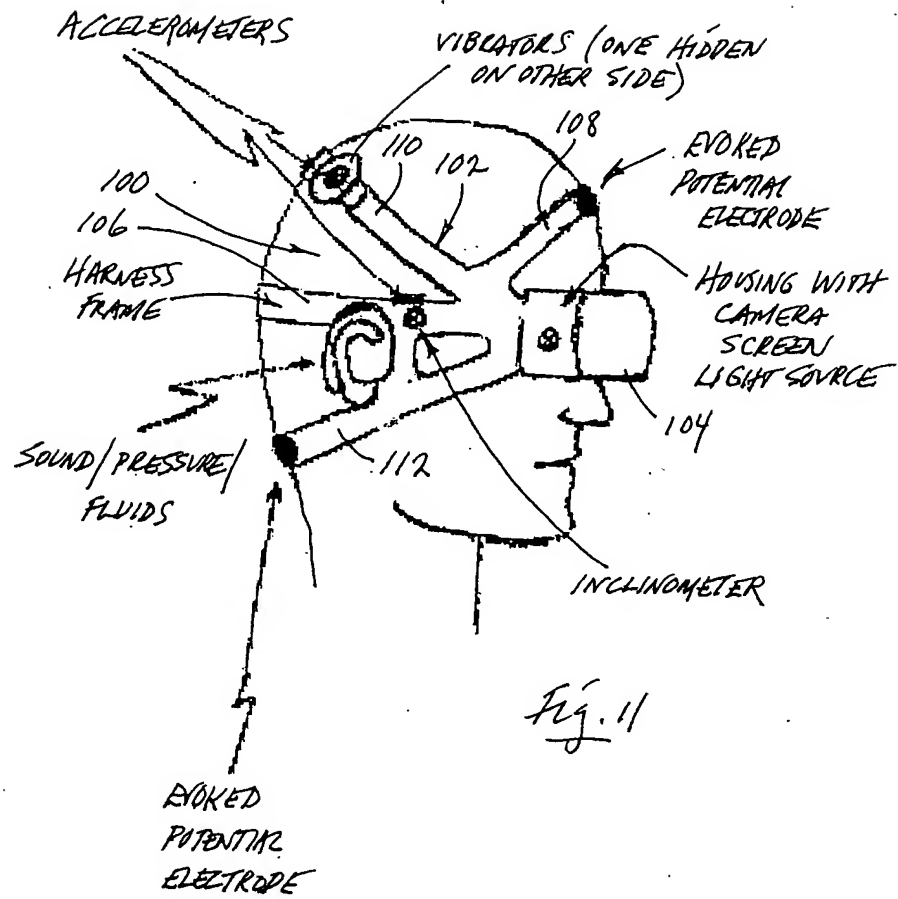


Fig. 11

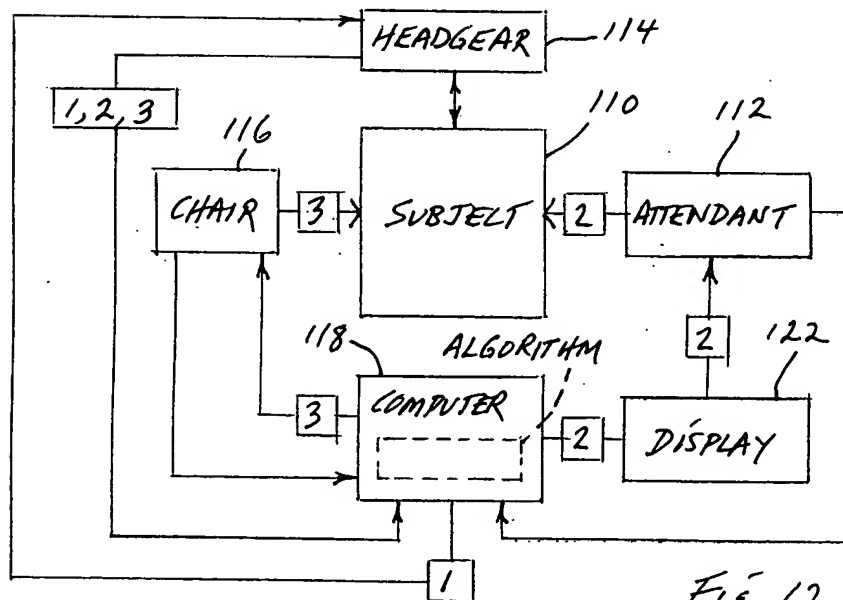


Fig. 12